Application Note · multi N/C 2100S





Challenge

Reproducible and reliable determination of TOC and TN_b contents in particle loaded wastewater samples.

Solution

Fully automated and simultaneous TOC/TN_b measurement using direct injection technology providing optimum particle handling and minimized carry-over.

TOC/TN_b Determination in Pulp and Paper Process Effluents

Introduction

The pulp and paper industry generates large volumes of wastewater or effluents that need to be treated before they can be reused or released into natural waterways.

According to the European Industrial Emissions Directive (IED) Best Available Techniques (BAT) have to be implemented within the EU for direct wastewater discharges from pulp, paper and card production¹⁾. The BAT reference document (BREF) indicates that among other parameters, TOC (total organic carbon) and TN_b (total bound nitrogen) are of growing importance. They need to be monitored on a daily or weekly basis. Furthermore, for economic and environmental reasons a preference for the parameter TOC instead of COD is given as it does not require the use of highly toxic compounds like dichromate (Cr VI) and mercury.

In many cases the COD and TN contents are still measured using separate methods. This is a labour and time consuming process and associated with the formation of chromium VI and mercury contaminated waste. By correlation studies an empirical conversion factor for TOC (total organic carbon) to COD conversion can be established for specific emission sources and waste water treatment steps. This allows a fully automated analysis process for TOC/TN_b determination according to EN 1484 and EN 12260 (as well as the planned new ISO 20236 for both parameters) to be applied, which saves resources and time.



Since process effluents from pulp and paper production often contain a large amount of solids (cellulose fibers), direct injection technology has proven particularly effective for TOC/TN, analysis. The multi N/C 2100S does not require hoses or valve technology, but doses the sample directly into the combustion chamber via a septum-free injection port and a wide bore needle using a microliter syringe. The direct injection technique provides a safe and reproducible particle transfer without the risk of clogging or carryover. This increases instrument availability, reduces wear and tear and increases sample throughput and efficiency.

Materials and Methods

Samples and Reagents

- Samples from different product processing and clean-up stages as well as raw water used in production were analyzed
- 2 M HCl was used for automatic acidification in NPOC mode

Sample Preparation and measurement

The samples were stored in a refrigerator at 4 °C until analysis. For measurement, the samples were transferred into 8 ml autosampler vials. The wastewater samples were analyzed in direct mode using an NPOC/TN method. The sampler AS 60 with 60 sample positions was used for automated measurement.

The samples were automatically acidified to a pH <2 using 2 M HCl, and subsequently purged to remove any inorganic carbon (TIC). The complete TIC elimination from the sample can be checked by TIC control measurement. A representative injection volume of 500 µL was transferred into the combustion tube for measurement. The samples were completely oxidized at a temperature of 800 °C in an oxygen-rich atmosphere using a platinum catalyst. The formed CO, was quantitatively determined by focus radiation none-dispersive infrared detection (FR-NDIR). Simultaneously the nitrogen oxides were detected by means of an electrochemical ChD detector (alternatively, chemiluminescence detector can be used for total bound nitrogen (TN_b) determination.

Calibration

Within the method up to 3 calibration ranges can be linked to each parameter in order to cover an over-all working range of up to 3 magnitudes. Detection limits and limits of quantification are depending on the selected working range and can be derived from the method characteristics given above.

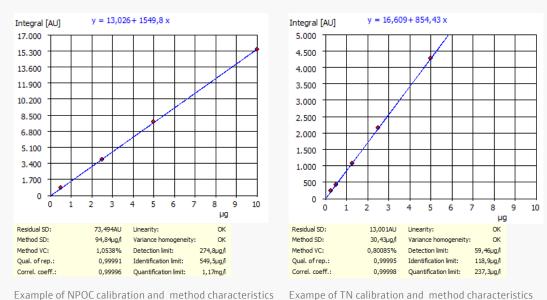


Table 1: NPOC and TN_b calibration curves

Exampe of TN calibration and method characteristics

Within one method up to three calibration ranges can be linked to each parameter in order to cover an over-all working range of up to three magnitudes. Detection limits and limits of quantification are depending on the selected working range and can be derived from the method characteristics given above.

Instrumentation

The analysis was performed on a multi N/C 2100S using an NPOC/TN method.

Method Parameters

The following method settings were used to determine the NPOC and TN_{h} contents:

Table 2:

| Parameter | multi N/C 2100S | | |
|------------------------------------|---|--|--|
| Measurement parameter | NPOC / TN _b | | |
| Digestion | High temperature digestion at 800 °C with platinum catalyst | | |
| Number of repetitions | min. 2, max. 3 | | |
| Rinse with sample before injection | 3 times | | |
| Sample purge time | 300 sec. | | |
| Injection volume | 500 μl | | |


Results and Discussion


Table 3 shows blank value corrected mean values from at least two repeat measurements for different real samples and recoveries for TOC and TN_b reference solutions. Dilution ratios are also reported. For informative purposes, the COD contents provided for the respective samples and the TOC-COD correlation factors calculated from them were also given.


Table 3:

| Sample ID | COD | NPOC ± RSD [mg/L] ± [%] | TN _b ± RSD [mg/L] ± [%] | TOC-COD correlation factor | Dilution factor |
|--|------|-------------------------|------------------------------------|----------------------------|-----------------|
| Raw Water | 8,0 | 2.79 ± 1.84 | 3.50 ± 1.02 | 2.86 | - |
| EVII | 8,9 | 2.99 ± 0.71 | 3.49 ± 0.68 | 2.98 | - |
| EX | 365 | 120.5 ± 0.18 | 4.60 ± 0.26 | 3.04 | - |
| ZF | 4302 | 1480 ± 0.08 | 15.36 ± 1.89 | 2.91 | 1:10 |
| Sedimat | 4450 | 1580 ± 0.47 | 15.50 ± 0.08 | 2.82 | 1:10 |
| ZA | 365 | 1600 ± 0.04 | 39.63 ± 1.33 | 3.17 | 1:10 |
| AA | 4302 | 956.5 ± 2.01 | 55.05 ± 1.66 | 3.27 | 1:10 |
| ВК | 4450 | 3230 ± 0.10 | 11.97 ± 2.18 | 2.55 | 1:100 |
| Check Standard Nicotinic Acid (TOC 20.0 / TN | 365 | 20.2 ± 0.9 | 3.97 ± 0.8 | _ | _ |

365 (TOC 20.0 / TN_b 3.88)

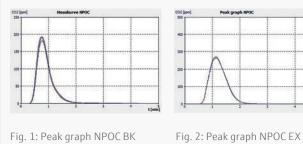








Fig. 3: Peak graph TN_b BK

Fig. 4: Peak graph TN_b EX

Conclusion

The analyzed samples represent a typical range of process effluents from different process stages and sampling points in the wastewater treatment process as well as raw water for paper production. Despite the very different TOC and TN_b concentrations, all samples were measured with outstanding accuracy and precision. Nicotinic acid was used as an analytical quality assurance standard (AQA) to simultaneously check for TOC and TN_b recoveries. Very good recoveries were achieved with this reference material for organically bound nitrogen.

This outstanding performance of multi N/C analyzers for such demanding wastewater matrices is based on the optimized combustion process with freely selectable combustion temperatures up to 950 °C. The direct injection with a septum-free pneumatic injection head in combination with a wide-bore needle of 0.7 μ m inner diameter, as well as proper sample homogenization on the auto sampler rack and the valve- and tubing-free sample transfer into the combustion system contribute to this. An operation mode keeping the stainless steel injection needle in the oven head at elevated temperatures during peak integration time to assure complete evaporation of TOC components and a clean needle for further sample processing in combination with an effective rinsing of the microliter injection syringe minimize carry-over effects.

A high degree of automation combined with the well-proven self-check system for trouble free unattended system operation make light work of TOC/TN_b analyses, even in challenging samples. In addition, the patented VITA flow management system compensates flow fluctuations inside the system caused by sample evaporation, providing TOC calibration stability for up to one year and saving valuable measurement time.

The analyzers of the multi N/C series are most suitable for the determination of total organic carbon and total bound nitrogen in process effluents and wastewater from pulp and paper industries.

References

1) Official Journal of the European Union, L 284/76, 30.09.2014, Commission Implementing Decision of 26. September 2014 "Establishing best available techniques (BAT) conclusions, under Directive 2010/75/EU of the European Parliament and of the Council, for the production of pulp, paper and board"

This document is true and correct at the time of publication; the information within is subject to change. Other documents may supersede this document, including technical modifications and corrections.

Headquarters

Analytik Jena AG Konrad-Zuse-Strasse 1 07745 Jena · Germany Phone +49 36 41 77 70 Fax +49 36 41 77 92 79 info@analytik-jena.com www.analytik-jena.com en \cdot 11/2018 © Analytik Jena AG | Picture p.1 © Istock/hxdyl Printout and further use permitted with reference to the source.